

بۆ گشت كۆمپانىياكانى ئاممىرى پزىشكى

الى كافة الشركات الاجهزة الطبية

م/پيشكه شكردنى ئۆفەر

عروض للاجهزة الطبية

تكايه ئۆفهرى خۇتان پيشكهش بكهن بۆ ئهم ئاممىره پزىشكيانهى خوارده به مهررجى نهوهى ولاىى
به رهه مهينهرى ئاممىرهكان (يابانى و نهوروبى و نه مريكى) بىت و ماوهى و مرهنتى له دوو سال
به رهو سه رهوه بىت .

يرجى تقديم عروضكم لقسم الاجهزة الطبية الواردة في الجدول ادناه على ان تكون الاجهزة من المنشأ)
اوروبا الغربية ، ياباني ، امريكي، مع تقديم ضمان لمدة سنتين فما فوق.

ND: YAG Laser 1.Q switched ND YAG 2.Energy: from 0.5md to 10md minimum 3.slit lamp with electric table a.slit lamp:should be compatible to receive SLT laser in future either from the same manufacturer or from others. The platform should be upgradable to become a 2in1 device: YAG+SLT laser platform The slit lamp should at least 3 manifactions. b-table: easy access electric table design for wheelchaired patients and of mobile type table. 4.power requirements:compatible to iraqi standards single phase,250v,50,60 hz 5.protective goggles for 1064nm wavelength	OCT Minimum required specification 1-should has both retinal and corneal (anterior segment)modules. 2-should has protocols for analysis of both macula and optic nerve head. 3-should be using spectral domain technology or newer technologies. 4-easy access design of its electric table for wheel chaired patients and of mobile type table. 5-power requirements be comptable with Iraqi standards and single phase 6-DICOM compatible	Ophthalmic operation microscope Minimum required specifications 1-motorized zoom,motorized focusing with apochromatic lens 2-assistant microscope (integrated or not)which can be controlled independently from main microscope 3-xy-coupling :motorized.big travel ranges are preferred 4-slit lamp equipped. 5-light:LED or xenon preferred,back up light source. 6-magnetic breaks for positioning . 7- Foot control :multifunction,wireless or not 8-coaxial illumination type 9-retro illumination booster system preferred 10-type of microscope: The microscope should be a professional microscope for anterior segment,cataract and retinal surgery.it should be of
---	--	---

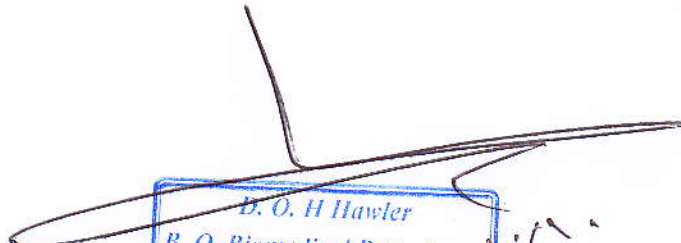
		floor type. 11-accessories required: a-full range of accessories required for retinal surgery whether standard or optional ones. b-keratoscope whether integrated or added as optional system. c-full system of digital HD video and image capturing unit and monitor d-slit lamp(already mentional)
--	--	---

تکایه ریزبهندی نامیرهکه به گویرهی ئەم راگهیانندنه بیت لهسهه ئۆفهر . وه ههر برکهیهک به تهنیا پیشکەش بکریت به دیناری عیراقی ، وه ئۆفهرهکان پیشکەشی بهشی نامیری پزشکی دهکریت لهگهڵ نوسینی ناوی نامیر و ژمارهکی .

دووا مۆلەت بۆ پیشکەش کردن 27/10/2013

یرجی تدوین تسلسل الجهاز بالاعلان على العرض، وتقديم عرض كل فقرة على حدى، تقديم الاسعار بالدينار العراقي. يتم تقديم العروض مباشرة الى قسم الاجهزة الطبية مع كتابة اسم ورقم الشركة

آخر موعد للتقديم 27/10/2013


 D. O. H Hawler
 B. O. Biomedical Department
 Eng. Pola Saudi Ali